



SZABO SCANDIC

Part of Europa Biosite

Produktinformation



Forschungsprodukte & Biochemikalien



Zellkultur & Verbrauchsmaterial



Diagnostik & molekulare Diagnostik



Laborgeräte & Service

Weitere Information auf den folgenden Seiten!
See the following pages for more information!



Lieferung & Zahlungsart

siehe unsere [Liefer- und Versandbedingungen](#)

Zuschläge

- Mindermengenzuschlag
- Trockeneiszuschlag
- Gefahrgutzuschlag
- Expressversand

SZABO-SCANDIC HandelsgmbH

Quellenstraße 110, A-1100 Wien

T. +43(0)1 489 3961-0

F. +43(0)1 489 3961-7

mail@szabo-scandic.com

www.szabo-scandic.com

[linkedin.com/company/szaboscandic](https://www.linkedin.com/company/szaboscandic) 



6042 Cornerstone Court W, Ste B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

Data Sheet

CD47:SIRP- γ [Biotinylated] Inhibitor Screening Assay Kit

Catalog # 72059

Size: 96 reactions

BACKGROUND: Signal-regulatory protein gamma (SIRP- λ), also known as CD172g, is a cell surface protein expressed mainly by myeloid cells such as macrophages. Its receptor, CD47, is ubiquitously expressed on the surface of all cells and has been found to be overexpressed in some cancers. CD47 binding to SIRP- λ has been shown to be important for T cell trans-endothelial migration (TEM).

DESCRIPTION: The *CD47:SIRP- γ [Biotinylated] Inhibitor Screening Assay Kit* is designed for screening and profiling inhibitors of CD47:SIRP- γ signaling. This kit comes in a convenient 96-well format, with biotin-labeled SIRP- γ (CD172g), purified CD47, streptavidin-labeled HRP, and assay buffer for 100 binding reactions. The key to this kit is the high sensitivity of detection of biotin-labeled SIRP- γ through streptavidin-HRP. Only a few simple steps on a microtiter plate are required for the assay. First, CD47 is coated on a 96-well plate. Next, SIRP- γ is incubated with CD47 on the plate. Finally, the plate is treated with streptavidin-HRP followed by addition of an HRP substrate to produce chemiluminescence, which can be measured using a chemiluminescence reader.

COMPONENTS:

Catalog #	Component	Amount	Storage	
71236	SIRP- γ , Biotin-labeled	5 μ g	-80°C	(Avoid freeze/thaw cycles!)
71177	CD47	10 μ g	-80°C	
79742	Streptavidin-HRP	15 μ l	+4°C	
79311	3x Immuno Buffer 1	50 ml	-20°C	
79728	Blocking Buffer 2	50 ml	+4°C	
79670	ELISA ECL substrate A (transparent bottle)	6 ml	RT	
	ELISA ECL substrate B (brown bottle)	6 ml	RT	
79699	White 96-well microplate	1	+4°C	

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**

Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Court W, Ste B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

MATERIALS OR INSTRUMENTS REQUIRED BUT NOT SUPPLIED:

PBS (Phosphate buffered saline)

Luminometer or fluorescent microplate reader capable of reading chemiluminescence

Rotating or rocker platform

APPLICATIONS: This kit is useful for screening for inhibitors of SIRP- γ binding to CD47.

STABILITY: One year from date of receipt when stored as directed.

REFERENCES:

1. Stefanidakis, *et al.*, *Blood*. 2008, **112(4)**:1280-1289
2. Sick, E., *et al.* *Br J Pharmacol*. 2012, **167(7)**:1415-1430.

ASSAY PROTOCOL:

All samples and controls should be tested in duplicate.

Coating the plate with CD47:

- 1) Thaw **CD47** on ice. Upon first thaw, briefly spin tube containing **CD47** to recover the full contents of the tube. Aliquot into single use aliquots. Immediately store remaining CD47 in aliquots at -80°C. *Note: CD47 is very sensitive to freeze/thaw cycles. Avoid multiple freeze/thaw cycles.*
- 2) Dilute **CD47** to 2 $\mu\text{g/ml}$ in PBS.
- 3) Add 50 μl of diluted **CD47** solution to each well and incubate overnight at 4°C. Leave a couple of wells empty (uncoated), for use with the "Ligand Control" (see below).
- 4) Dilute **3x Immuno Buffer 1** to **1x Immuno Buffer 1** with water. Dilute only enough **3x Immuno Buffer 1** required for washing the plate (below).
- 5) Decant to remove supernatant. Wash the plate 3 times with 100 μl **1x Immuno Buffer 1**. Tap plate onto clean paper towels to remove liquid.
- 6) Block wells by adding 100 μl of **Blocking Buffer 2** to each well. Incubate for 1 hour at room temperature. Remove supernatant as described in step 4.

Step 1:

- 1) Prepare the master mixture: N wells \times (10 μl **3x Immuno Buffer 1** + 15 μl H₂O).

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**

Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Court W, Ste B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

- 2) Add 25 μ l of master mixture to each well. Use uncoated wells for the “Ligand Control”.
- 3) Add 5 μ l of inhibitor solution to each well designated “Test Inhibitor”. For the “Positive Control”, “Ligand Control”, and “Blank”, add 5 μ l of the same solution without inhibitor (inhibitor buffer). Incubate at room temperature for one hour.
- 4) Thaw **SIRP- γ -biotin** on ice. Upon first thaw, briefly spin tube containing enzyme to recover full contents of the tube. Aliquot **SIRP- γ -biotin** into single use aliquots. Immediately store remaining undiluted enzyme in aliquots at -80°C . *Note: SIRP- γ -biotin is very sensitive to freeze/thaw cycles. Do not re-use thawed aliquots or diluted enzyme.*

	Blank	Ligand Control	Positive Control	Test Inhibitor
3x Immuno Buffer 1	10 μ l	10 μ l	10 μ l	10 μ l
H ₂ O	15 μ l	15 μ l	15 μ l	15 μ l
Test Inhibitor/Activator	-	-	-	5 μ l
Inhibitor buffer (no inhibitor)	5 μ l	5 μ l	5 μ l	-
1x Immuno Buffer 1	20 μ l	-	-	-
SIRP- γ -biotin (2 μ g/ml)	-	20 μ l	20 μ l	20 μ l
Total	50 μl	50 μl	50 μl	50 μl

- 5) Dilute **SIRP- γ -biotin** to 2 μ g/ml in **1x Immuno Buffer 1**. Keep diluted protein on ice until use. Discard any unused diluted protein after use.
- 6) Add 20 μ l of **1x Immuno Buffer 1** to the well designated “Blank”.
- 7) Initiate reaction by adding 20 μ l of diluted **SIRP- γ -biotin** (see Step 1-5) to wells labeled “Positive Control”, “Ligand Control” and “Test Inhibitor”. Incubate at room temperature for two hours.
- 8) Decant to remove supernatant. Wash the plate three times with 100 μ l/well **1x Immuno Buffer 1**. Tap plate onto clean paper towels to remove liquid.
- 9) Block wells by adding 100 μ l of **Blocking Buffer 2** to each well. Incubate for 10 minutes at room temperature. Remove supernatant as in Step 1-8.

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**

Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Court W, Ste B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

Step 2:

- 1) Dilute **Streptavidin-HRP** 1000-fold with **Blocking Buffer 2**.
- 2) Add 100 μ l to each well. Incubate for 1 hour at room temperature with slow shaking.
- 3) Wash plate three times with **1x Immuno Buffer 1**. Tap plate onto clean paper towels to remove liquid.
- 4) Block wells by adding 100 μ l of **Blocking Buffer** to each well. Incubate for 10 minutes at room temperature. Decant to remove supernatant. Tap plate onto clean paper towels to remove liquid.
- 5) Just before use, mix on ice 50 μ l **ELISA ECL Substrate A** and 50 μ l **ELISA ECL Substrate B**, then add 100 μ l to each well. Discard any unused chemiluminescent reagent after use.
- 6) Immediately read sample in a luminometer or microtiter-plate capable of reading chemiluminescence. "Blank" value is subtracted from all readings.

Reading Chemiluminescence:

Chemiluminescence is the emission of light (luminescence) which results from a chemical reaction. The detection of chemiluminescence requires no wavelength selection because this method uses emission photometry and is not emission spectrophotometry.

To properly read chemiluminescence, make sure the plate reader is set for LUMINESCENCE mode. Typical integration time is 1 second; delay after plate movement is 100 msec. Do not use a filter when measuring light emission. Typical settings for the Synergy 2 BioTek plate reader are: use the "hole" position on the filter wheel; Optics position: Top; Read type: endpoint. Sensitivity may be adjusted based on the luminescence of a control assay without enzyme (typically we set this value as 100).

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**


Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Court W, Ste B
 San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

Example of Assay Results:

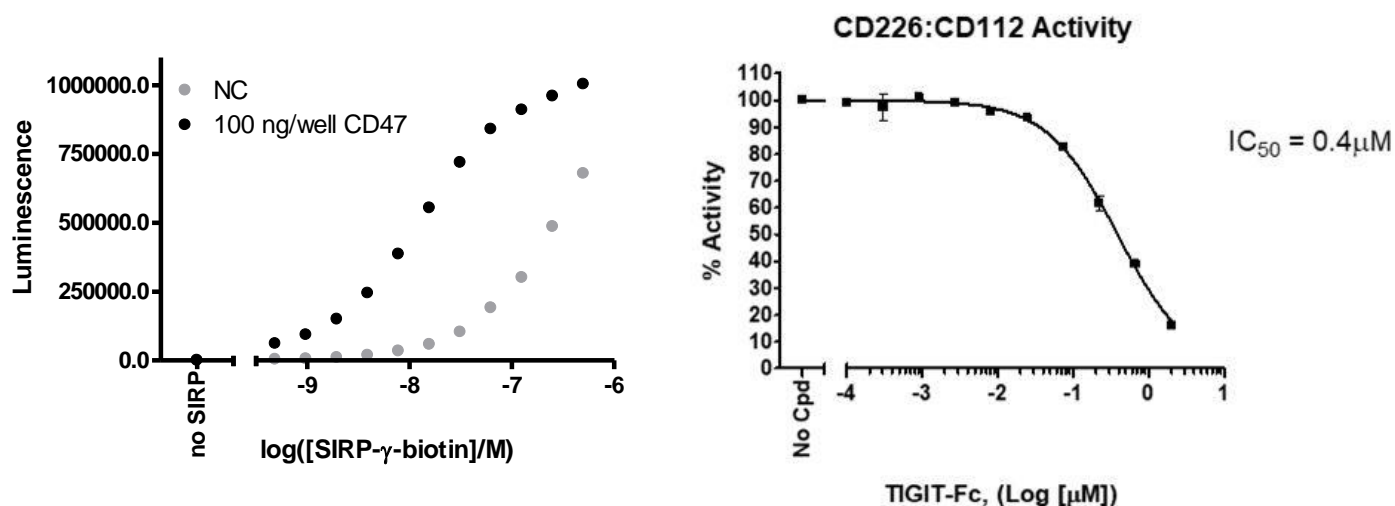

(Left) Interaction of CD47 with SIRP-γ-biotin using the *CD47:SIRP-γ[Biotinylated] Inhibitor Screening Assay Kit*, BPS Bioscience, Catalog #72059 (non-coated wells, NC). (Right) Inhibition of CD47:SIRP-γ interaction by SIRP-α. *Data shown is lot-specific. For lot-specific information, please contact BPS Bioscience, Inc. at info@bpsbioscience.com.*

RELATED PRODUCTS:

<u>Product Name</u>	<u>Catalog #</u>	<u>Size</u>
CD47, Fc fusion	71177	100 μg
CD47, Fc fusion, Biotin-labeled	71169	50 μg
CD47, His-tag	71127	100 μg
SIRP-α, His-tag	71145	100 μg
SIRP-α, His-tag, Biotin-labeled	71138	50 μg
SIRP-γ (CD172g), Fc fusion, Biotin-labeled	71236	50 μg
CD47:SIRP-α[Biotinylated] Inhibitor Screening Assay Kit	72044	96 rxns

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**
 Or you can Email us at: info@bpsbioscience.com
 Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Court W, Ste B
 San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

TROUBLESHOOTING GUIDE

Problem	Possible Cause	Solution
Luminescence signal of positive control reaction is weak	CD47 or SIRP- γ has lost activity	Enzyme loses activity upon repeated freeze/thaw cycles. Use fresh SIRP- γ -biotin, (BPS Bioscience #71236) and fresh CD47 (BPS Bioscience #71177). Store proteins in single-use aliquots. Increase time of enzyme incubation. Increase enzyme concentration.
	Incorrect settings on instruments	Refer to instrument instructions for settings to increase sensitivity of light detection.
	Chemiluminescent reagents mixed too soon	Chemiluminescent solution should be used within 15 minutes of mixing. Ensure both reagents are properly mixed.
Luminescent signal is erratic or varies widely among wells	Inaccurate pipetting/technique	Run duplicates of all reactions. Use a multichannel pipettor. Use master mixes to minimize errors.
	Bubbles in wells	Pipette slowly to avoid bubble formation. Tap plate lightly to disperse bubbles; be careful not to splash between wells.
Background (signal to noise ratio) is high	Insufficient washes	Increase number of washes. Increase wash volume. Increase Tween-20 concentration to 0.1% in PBST.
	Sample solvent is inhibiting the enzyme	Run negative control assay including solvent. Maintain DMSO level at <1% Increase time of enzyme incubation.
	Results are outside the linear range of the assay	Use different concentrations of SIRP- γ -biotin (BPS Bioscience #71236) to create a standard curve.

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**

Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com