



SZABO SCANDIC

Part of Europa Biosite

Produktinformation



Forschungsprodukte & Biochemikalien



Zellkultur & Verbrauchsmaterial



Diagnostik & molekulare Diagnostik



Laborgeräte & Service

Weitere Information auf den folgenden Seiten!
See the following pages for more information!



Lieferung & Zahlungsart

siehe unsere [Liefer- und Versandbedingungen](#)

Zuschläge

- Mindermengenzuschlag
- Trockeneiszuschlag
- Gefahrgutzuschlag
- Expressversand

SZABO-SCANDIC HandelsgmbH

Quellenstraße 110, A-1100 Wien

T. +43(0)1 489 3961-0

F. +43(0)1 489 3961-7

mail@szabo-scandic.com

www.szabo-scandic.com

[linkedin.com/company/szaboscandic](https://www.linkedin.com/company/szaboscandic) 

Elite™ Glucose Colorimetric/Fluorometric Assay Kit

CATALOG NUMBER: CA-G005, 500 assays (5x 96-well plate)

Description

Glucose (C₆H₁₂O₆) is a ubiquitous fuel in biology. It is used as an energy source in most organisms, from bacteria to humans. Glucose level is a key diagnostic parameter for many metabolic disorders, such as diabetes.

The Elite™ Glucose assay kit provides a quick and sensitive method for the measurement of glucose. It uses glucose oxidase-based enzyme coupled reactions to detect glucose through the production of hydrogen peroxide, which is monitored by our Elite™ peroxidase substrate. Elite™ peroxidase substrate can be recorded in a dual mode: colorimetric assay at 570 nm and fluorometric assay at Ex/Em = 540/590 nm. The assay is robust, and can be readily adapted for a wide variety of applications that require the measurement of glucose. The assay has very low background since it is run in the red visible range that significantly reduces the interference from biological samples. It has demonstrated high sensitivity and low interference with excitation at 570 nm and emission at 590 nm. When using fluorometric detection, we can detect as little as 3 μM D-glucose.

Kit Components

- | | |
|---|--------------------|
| • Component A: Elite™ Peroxidase Substrate (light sensitive) | 1 vial |
| • Component B: Assay Buffer | 1 bottle (50 ml) |
| • Component C: Horseradish Peroxidase (HRP) | 1 vial (10 units) |
| • Component D: Glucose Oxidase | 1 vial (100 units) |
| • Component E: DMSO | 1 vial (200 μl) |
| • Component F: Glucose Standard | 1 vial (144 mg) |

Storage

Keep **Component A** at -20 °C and avoid exposure to light; **Component C&D** at -20 °C; **Component B, E&F** at 4 °C. All components are stable for 6 months after receipt if stored properly.

Shelf Life

All reagents are stable for 6 month after receipt when stored properly at the recommended conditions.


Materials Required (but not supplied)

- 96 microplates: Tissue culture microplate with black wall and clear bottom is recommended.
- Fluorescence microplate reader.



Assay Protocol

Summary of the Assay

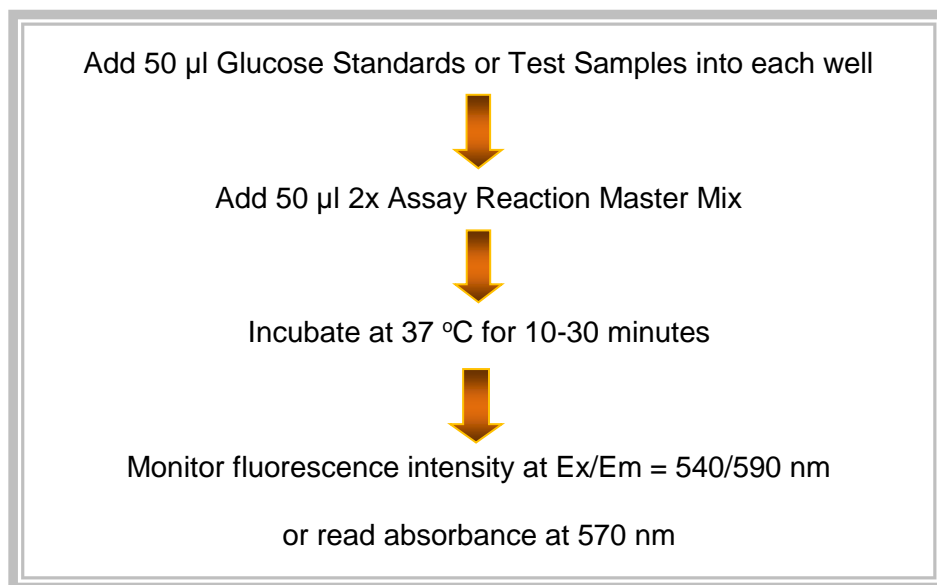

1. Preparation of Stock Solutions:

1.1 250x Elite™ Peroxidase Substrate Stock Solution: Add 100 µl of DMSO (**Component E**) into the vial of Elite™ Peroxidase Substrate (**Component A**) to make 250x Elite™ Peroxidase Substrate stock solution.

Note: The unused 250x Elite™ Peroxidase Substrate stock solution should be divided into single use aliquots and stored at -20 °C.

Note: The Elite™ Peroxidase Substrate is unstable in the presence of thiols such as dithiothreitol (DTT) and 2-mercaptoethanol. The final concentration of DTT or 2-mercaptoethanol in the reaction should be no higher than 10 µM. The Elite™ Peroxidase Substrate is also unstable at high pH (>8.5). Therefore, the reaction should be performed at pH7-8. The provided assay buffer (pH 7.4) is recommended.

1.2 HRP Stock Solution (10 U/ml): add 1 ml of assay buffer (**Component B**) into the vial of horseradish peroxidase (**Component C**).

Note: the unused HRP solution should be divided into small aliquots and kept at -20 °C.

1.3 Glucose Oxidase Solution (100 U/ml): add 1 ml of assay buffer (**Component B**) into the vial of glucose oxidase (**Component D**).

Note: the unused glucose oxidase solution should be divided into small aliquots and kept at -20 °C.

1.4 Glucose Standard Stock Solution (800 mM): add 1 ml of assay buffer (**Component B**) into the vial of glucose standard (**Component F**).

Note: the unused glucose standard solution should be kept at -20 °C.

2. Preparation of Assay Reaction Master Mix:

Prepare Assay Reaction Master Mix (2x) according to the Table 1 (protected from light).

Table 1. Assay Reaction Master Mix (2x) for one 96-well plate

Components	Volume
250x Elite™ Peroxidase Substrate Stock Solution (from Step 1.1)	20 µl

Data Analysis

The fluorescence in blank wells (with the assay buffer only) is used as a control, and subtracted from the values of those wells with the glucose reactions. A glucose standard curve is shown in Figure 1.

Note: The fluorescence background increases with time, thus it is important to subtract the fluorescence intensity value of the blank wells for each data point.

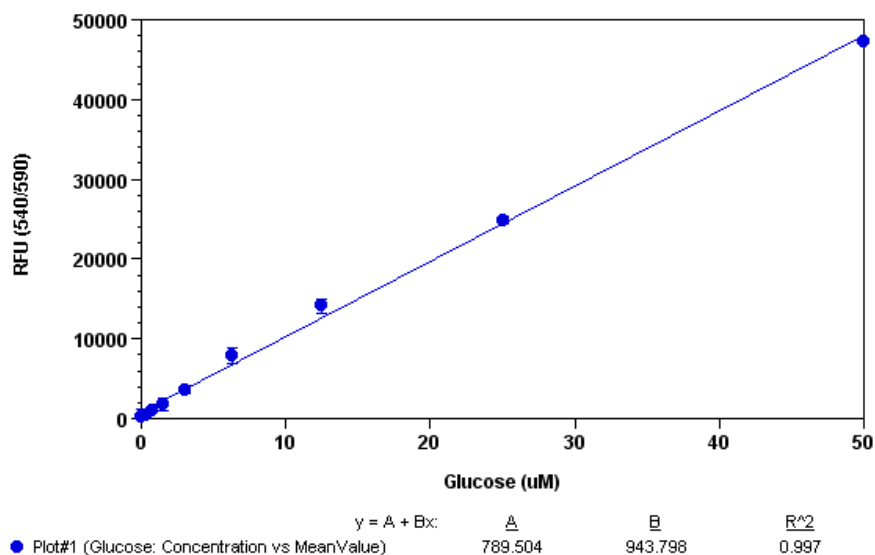


Figure 1. Glucose dose response was measured with Elite™ Glucose Colorimetric/Fluorimetric Assay Kit on a 96-well black plate using a Novostar microplate reader. As low as 3 µM glucose was detected with 30 minutes' incubation (n = 3).

Appendix A

Sample lysis preparation for the assay kits

This protocol serves as a general guide for preparing samples for the assays. For the best results, users need to adjust the amount of materials for their unique cell samples.

1. Lysis of plant cells

Homogenize the leaves with the lysis buffer (Cat# CA-N015g) at 200 mg/ml, and centrifuge at 2500 rpm for 5-10 minutes. Use the supernatant for the assay.

2. Lysis of bacterial cells

Collect bacterial cells by centrifugation (i.e. 10,000 x g, 0°C, 15min). Add lysis buffer (Cat# CA-N015g) to the pellet (1 mL per 100 to 10,000,000 cells), and leave at room temperature for 15 minutes. Centrifuge at 2500 rpm for 5 minutes, and use the supernatant for the assay.

3. Lysis of mammalian cells

Remove the medium from the culture plate (wells). Use about 100 µL lysis buffer (Cat# CA-N015g) per 1-5 million cells (or add lysis buffer 100 µL lysis buffer per well in a 96-well cell culture plate), and leave at room temperature for 15 minutes. For the assay, use the lysate directly or centrifuge at 1500 rpm for 5min then use the supernatant.

4. Lysis of tissues

Weigh ~ 20 mg tissue, then wash with cold PBS buffer. Homogenize the tissue with 400 µl of lysis buffer (Cat# CA-N015g) in a micro-centrifuge tube, and centrifuge at 2500 rpm for 5-10 minutes. Use the supernatant for the assay.

