



SZABO SCANDIC

Part of Europa Biosite

Produktinformation



Forschungsprodukte & Biochemikalien



Zellkultur & Verbrauchsmaterial



Diagnostik & molekulare Diagnostik



Laborgeräte & Service

Weitere Information auf den folgenden Seiten!
See the following pages for more information!



Lieferung & Zahlungsart

siehe unsere [Liefer- und Versandbedingungen](#)

Zuschläge

- Mindermengenzuschlag
- Trockeneiszuschlag
- Gefahrgutzuschlag
- Expressversand

SZABO-SCANDIC HandelsgmbH

Quellenstraße 110, A-1100 Wien

T. +43(0)1 489 3961-0

F. +43(0)1 489 3961-7

mail@szabo-scandic.com

www.szabo-scandic.com

[linkedin.com/company/szaboscandic](https://www.linkedin.com/company/szaboscandic) 

Urinary Tract infection (UTI) - A Rapid Screen

**For both doctors' offices
and laboratories**

- ▶ Indicates UTI within 2 minutes
- ▶ Visual detection
- ▶ Easy to use and needs no instruments
- ▶ Can be used by untrained personnel in outpatient settings
- ▶ Improved performance as compared with routine urinalysis
- ▶ Exceptionally sensitive for low bacterial counts
(5×10^4 CFU/ml at 93% sensitivity)
- ▶ Screening out negative specimens, eliminates the need
for prolonged culture procedure
- ▶ Early diagnosis prevents unnecessary treatment and minimizes costly
complications of UTI



Uriscreen™

- ▶ **Uriscreen™** is a rapid screening test which combines the detection of both bacteriuria and pyuria (the presence of somatic cells in urine), by detecting catalase activity (an enzyme present in many eukaryotic cells).
- ▶ **Uriscreen™** provides physicians' offices, clinical laboratories and outpatient sites with the ability to provide fast and accurate screening for urinary tract infections.
- ▶ **Uriscreen™**'s negative predictive value (NPV) of at least 95%, was higher than the NPV of the dipstick (see references).
- ▶ **Uriscreen™** is a cost-effective, screening procedure which can be used to complement conventional culture methods.

Savyon Diagnostics has exclusive worldwide rights to the patented **Uriscreen™** technology.

Ordering information

Cat. Number	Product Name	Number of Tests
101-01	Uriscreen™	20

Also available in bulk format

References

1. Carroll K. C. et. al., 1994, "Laboratory Evaluation of Urinary Tract Infection in an Ambulatory Clinic", *Am. J. Clin. Pathol.*; 101:100-103.
2. Hagay, Z. et. al., "Uriscreen, a Rapid Enzymatic Urine Screening Test: Useful Predictor of Significant Bacteriuria in Pregnancy".

Procedure:



Urine specimen is added to a test tube ▼



4 drops of hydrogen peroxide solution are added to the tube and mixed ▼



The appearance of white foam indicates a positive result

Negative



Positive



Indicates presence of UTI (bacteriuria/hematuria/pyuria)

SAVYON DIAGNOSTICS Ltd.

3 Habosem St, Ashdod 77610, Israel
Tel: 972.8.8562920 Fax: 972.8.8523176
e-mail: info@savyondiagnosics.com
www.savyondiagnosics.com



URISCREEN™

Rapid UTI Screen test for bacteriuria and presence of somatic cells in urine

Instruction Manual

Test kit for 20 determinations
(Catalog no. 101-01)

For In Vitro Diagnostic Use
For professional use only
Store in a dark place at 10-28°C (50-82°F)

Savyon® Diagnostics Ltd.

3 Habosem St. Ashdod 77610
ISRAEL

Tel.: +972.8.8562920

Fax: +972.8.8523176

support@savyondiagnosics.com E-mail:

Intended Use

URISCREEN is a rapid screening test for UTI. The test is primarily intended for the screening of asymptomatic populations (e.g., routine testing in schools, industrial plants, institutions, hospitals, clinics, physicians' offices, etc.) for significant bacteriuria, hematuria, pyuria and the presence of other somatic cells in urine.

A POSITIVE RESULT INDICATES THAT THE URINE REQUIRES FURTHER LABORATORY EXAMINATION FOR MORE DETAILED DIAGNOSIS.

Precautions and Warnings

1. This kit contains a 10% hydrogen peroxide (H₂O₂) solution and a colored reagent powder which stains and may be irritating. Do not heat or mix with flammable substances. Avoid contact with eyes, skin and clothing. In case of such contact, flush immediately with a large volume of water.
2. Urine specimens should be treated as potentially infectious material.
3. The reagents in this kit have been standardized as a unit. No reagents should be used which are **outdated**, bear a **different lot number** from that imprinted on this kit, or are manufactured by **another manufacturer**.
4. The reagents included in this kit are for **in vitro diagnostic use only**.

Introduction

Urinary tract infections are considered to be among the most frequently occurring infectious diseases. Surveys have demonstrated that approximately 80% of the urine specimens cultured in clinical microbiology laboratories are either negative or contain no significant bacteriuria. The classical screening methods for bacterial contamination of urine are still

based on bacteriological culture plating, which generally requires a minimum of 24 hours, and is usually expensive.

The obvious need for faster and less costly screening methods for bacteriuria and other urinary tract anomalies – especially among asymptomatic populations – has led to the development of alternative techniques. Most are based on sensitive and specific staining procedures for various bacterial and somatic cell components, or on detecting the presence of intracellular molecules such as adenosine triphosphate and certain enzymes not usually present in healthy urine⁽¹⁻⁶⁾.

Catalase has been found to be present in many eukaryotic and prokaryotic cells⁽⁷⁻⁹⁾. In infected urine, it has been found in most bacteria that attack the urinary tract, as well as in inflammatory exudates cells⁽⁹⁻¹¹⁾. It is also present in high concentrations in kidney cells⁽¹⁷⁾.

Urine, which is normal, clean and healthy, has no significant catalase activity^(10, 11, 18). When detected by the **URISCREEN** test, catalase activity is indicative of significant bacteriuria (>5 x 10⁴ CFU/ml) and/or an abnormally high number of somatic cells (>10 per high power field), typically associated with infection, damage or other urinary tract pathology.

It is well recognized that the evaluation of asymptomatic urine specimens for infection should include **both bacteriuria and pyuria**, since in many cases results of high bacterial counts were found to be indicative **only when accompanied by a test for pyuria**⁽¹²⁻¹⁵⁾. This rationale has also led other manufacturers to combine screening tests for pyuria (e.g. leukocyte esterase test).

The URISCREEN test combines the detection of both bacteriuria and the presence of somatic cells in urine, in a single test which is extremely simple to perform, requires no equipment, is inexpensive and **can be completed and evaluated in about a minute**.

Principle of the Test

In the first step, the urine specimen is mixed with a test reagent powder which enables catalase detection. This step is fast, taking only a few seconds to complete.

In the second step, a small amount of hydrogen peroxide solution is added to the contents of the tube and mixed. The quantity of the resulting foam indicates the presence and relative level of catalase originating from bacterial and/or somatic cells in the urine. Lack of foam indicates negative test results.

Kit Contents

- 20 stoppered test tubes, with the test reagent powder. It is stable until the expiration date of the kit, providing the test tubes are stored unopened at room temperature.
- One dropper bottle containing 10 ml of 10% hydrogen peroxide (H₂O₂) solution. It is stable until the expiration date of the kit, providing it is stored the dark at room temperature.
- 20 disposable 2 ml pipettes
- Instruction manual

Materials Required But Not Supplied

- Negative control solution and impregnated discs for reconstitution of a positive control, (Catalog No. 104-01, available from Savyon Diagnostics Ltd.)

Quality Control Procedure

A positive and negative control must be run once upon opening a new lot.

Instructions for performing these controls are provided with the reagents needed (negative control solution and impregnated disks).

Note: *If the positive control does not yield an appropriate result, repeat the test, preferably with an impregnated disk from a new lot. If a proper result is not obtained, the test kit should not be used.*

Collection and Preparation of Specimens


Collect midstream urine in a clean container. Test as soon as possible. If the test cannot be performed within one hour after collection, the sample may be stored at 4°C (39°F) for not more than four hours.

Test Procedure

1. Transfer 1.5 – 2 ml of the urine to be tested into a provided test tube containing URISCREEN Reagent Powder. Use one test tube for each urine sample. Repeat this step for every specimen to be tested up to a maximum of 20 tubes “in one operation”.
2. Add four drops of URISCREEN 10% Hydrogen Peroxide Solution to each test tube. Mix gently, in order not to produce foam, for five seconds.
3. Watch for foam formation and monitor the results for 1-2 minutes after initiation of step 2. If the test is positive, foam will be formed on the surface of the liquid. Observe the foam, and then refer to the Result Interpretation (Figure 1).

Interpretation of Results

Figure 1

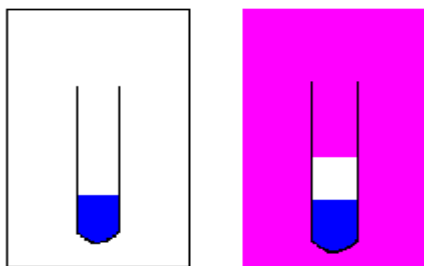

NEGATIVE

POSITIVE

Positive Results

Foam is generated at least to an extent sufficient to form a complete and continuous ring or layer on the surface of the liquid along the test tube walls.

The formation of foam indicates the presence of catalase in the urine (refer to Figure 1). A positive result indicates UTI. The urine of the patient should be further examined using more detailed procedures.

Negative Results

Either no foam whatsoever is generated, or the ring of foam remains incomplete at the end of two minutes.

Limitations of the Test

1. The **URISCREEN** test does not detect catalase – negative organisms, such as certain species of Streptococcus which occur in approximately 2% of all specimens screened, and 5-10% of those demonstrating positive results. However, about half of these species are detectable by the **URISCREEN** test **via the pyuria**, which was found to accompany about 50% of these infections.
2. As with all screening tests, definitive diagnostic or therapeutic decisions should not be based on any single method or result.
3. Specimens should be well mixed to ensure that a representative sample is tested.
4. A positive result indicates that the patient's urine should be subjected to more detailed examination.

Performance Characteristics

In a comparative study conducted during a six-month period, 2961 urine specimens from asymptomatic populations were randomly collected. Bacterial counts were determined by plating on MacConkey and blood agar plates; somatic cells were counted microscopically. In parallel, the specimens were also tested by the URISCREEN test; the results are presented in Table 1.

Table 1

Bacterial Counts (CFU/ml)	Somatic Cells	Results with URISCREEN	
		POSITIVE	NEGATIVE
<10,000	-	347	1426
	+	381	21
10,000-50,000	-	66	34
	+	70	10
>50,000	-	173	38
	+	378	17

Sensitivity, specificity and negative predictive value were calculated at two cutoff levels of bacterial counts: >10,000 CFU/ml and > 50,000 CFU/ml.

- A. Specimens with significant pyuria, hematuria or other somatic cells (>10 cells per high power field), as determined by microscopic counting, were considered as true positives even if bacterial counting showed less than 10,000 CFU/ml. The specimens containing <10,000 or <50,000 CFU/ml (depending on the cutoff level considered) without somatic cells were considered true negatives.

1. For bacteriuria cutoff level at >10,000 CFU/ml:

Sensitivity = 90%
 Specificity = 80%
 Negative Predictive Value = 92%

2. For bacteriuria cutoff level at >50,000 CFU/ml:

Sensitivity = 92%
 Specificity = 78%
 Negative Predictive Value = 94.5%

- B. Considering that evaluation of urine specimens for UTI should include both bacteriuria and pyuria⁽¹²⁻¹⁵⁾, only those specimens that contained >10,000 CFU/ml and >10 somatic cells per high power field were considered as true positives.

Sensitivity and negative predictive value are:

Sensitivity = 94%
 Negative Predictive Value = 98%

In another comparative study, 976 urine specimens were collected from asymptomatic populations. Bacterial counts were determined by counting on MacConkey and Cled agar plates on dip slides. Somatic cells were counted microscopically.

Table 2 depicts the results, compared with those obtained by the URISCREEN test.

Table 2

Bacterial Counts (CFU/ml)	Somatic Cells	Results with URISCREEN	
		POSITIVE	NEGATIVE
<50,000	-	95	462
	+	236	8
>50,000	+ and -	160	15

In calculating sensitivity, specificity and negative predictive value, specimens were considered negative if they showed less than 5×10^4 CFU/ml and/or less than 10 somatic cells per high power field.

The following results were obtained:

Sensitivity = 94%
 Specificity = 83%
 Negative Predictive Value = 95%

Bibliography

1. E. Bixler-Forell, M.A. Bertram and D.A. Bruckner: Clinical Evaluation of three rapid methods for the detection of significant bacteriuria, **Journal of Clinical Microbiology**, 22: 62-67 (1985).
2. T.C. Wu, E.C. Williams, S.Y. Koo and J.D. MacLowry: Evaluation of three bacteriuria screening methods in a clinical research hospital, **Journal of Clinical Microbiology**, 21: 796-799 (1985).
3. C.C. Longaria and G.A. Gonzalez: Filtra Check – UTI, a rapid disposable system for detection of bacteriuria, **Journal of Clinical Microbiology**, 25: 926-928 (1987).
4. P.R. Murry, T.B. Smith and T.C. McKinney Jr.: Clinical evaluation of three urine screening tests, **Journal of Clinical Microbiology**, 25: 467-470(1987).
5. H.O. Hollander, A. Kainer, A. Lundin and E. Osterberg: Evaluation of rapid methods for the detection of bacteriuria (screening) in primary healthcare, **Acta Path. Microbiol. Immunol. Scand., Section B**, 94: 39-49 (1986).
6. H.J. Cannon Jr., E.S. Goetz, A.C. Hamoudi and M.J. Marcon: Rapid screening and microbiologic processing of pediatric urine specimens, **Diagn. Microbiol. Infect. Dis.** 4: 7-11(1986).
7. G.R. Schonbaum and B. Chance, in **The Enzymes**, 2nd edition, P.D. Boyer, ed., Vol 13, pp. 363—408 (1976), Academic Press, New York.
8. V. Nadler, I. Goldberg and A. Hochman: Comparative study of bacterial catalases, **Biochim. et Biophys. Acta** 882: 234-241 (1986).
9. M.H. Fukami and T. Flatmark: Studies on catalase compartmentation in digitonin-treated rat hepatocytes, **Biochim. et Biophys. Acta** 889: 91-94 (1986).

10. K.A.J. Jarvinen: Determination of peroxidase in urine, **British Medical Journal**, 1: 379 (1958).
11. A.I. Braude and H.B. Pittsburgh: Detection of urinary catalase by disk flotation, **Journal Lab. And Clin. Med.** 57: 490-494 (1961).
12. M.A. Pfaller, G. Scharnweber, B. Stewart and F.P. Kuntz: Improved urine screening using a combination of leukocyte esterase and the Lumac system, **Diagn. Microbiol. Infect. Dis.** 3: 243-250 (1983).
13. M. Pfaller, B. Ringenberg, L. Rames, J. Hegeman and F.P. Kuntz: The usefulness of screening tests for pyuria in combination with culture in the diagnosis of urinary tract infection, **Diagn. Microbiol. Infect. Dis.** 6: 207-215 (1987).
14. G.V. Doern, M.A. Saubolle and D.I. Sewell: Screening of bacteriuria with the LN strip test, **Diagn. Microbiol. Infect. Dis.** 4: 355-358 (1986).
15. J.L. Staneck: Screening tests and rapid identification. Is anybody out there listening? **Diagn. Microbiol. Infect. Dis.** 3: 51S-57S (1985).
16. L.E. Collins, R.W. Clarke and R. Maskell: Streptococci as urinary pathogens, **The Lancet**, August 30, 479-481(1986).
17. I. Liberman and T. Ove: Enzyme activity levels in mammalian cell cultures, **J. Biol. Chem.** 223: 634-636 (1958).
18. A.I. Braude: Catalase activity of infected urine, **J. Clin. Inves.** 38: 990 (1959).



European Authorized Representative: Obelis s.a.
 Boulevard Général Wahis 53, B-1030 Brussels
 Tel: +32.2.732.59.54 Fax: +32.2.732.60.03
 E-mail: mail@obelis.net