



SZABO SCANDIC

Part of Europa Biosite

Produktinformation



Forschungsprodukte & Biochemikalien



Zellkultur & Verbrauchsmaterial



Diagnostik & molekulare Diagnostik



Laborgeräte & Service

Weitere Information auf den folgenden Seiten!
See the following pages for more information!



Lieferung & Zahlungsart

siehe unsere [Liefer- und Versandbedingungen](#)

Zuschläge

- Mindermengenzuschlag
- Trockeneiszuschlag
- Gefahrgutzuschlag
- Expressversand

SZABO-SCANDIC Handels GmbH

Quellenstraße 110, A-1100 Wien

T. +43(0)1 489 3961-0

F. +43(0)1 489 3961-7

mail@szabo-scandic.com

www.szabo-scandic.com

[linkedin.com/company/szaboscandic](https://www.linkedin.com/company/szaboscandic) 




savyonDIAGNOSTICS

member of the gamida diagnostics division

savvy•gen GI Bacteria Panel

REF 620-01L / 620-01H


Test kit for 48 determinations



For Professional Use Only



Savyon® Diagnostics Ltd.
3 Habosem St. Ashdod 7761003
ISRAEL
Tel.: +(972).8.8562920
Fax: +(972).8.8523176
E-mail: support@savyondiagnostics.com



**European Authorized
Representative: Obelis s.a.**
Boulevard Général Wahis 53
1030 Brussels, BELGIUM
Tel: +(32) 2. 732.59.54
Fax: +(32) 2.732.60.03
E-Mail : mail@obelis.net



Intended Use

The Savvygen™ GI Bacteria Panel allows the qualitative detection and differentiation of *Salmonella*, *Campylobacter* and *Shigella*/enteroinvasive *Escherichia coli* (EIEC) by R PCR in human stool specimens. The product is intended for use in the diagnosis of *Salmonella*, *Campylobacter* and/or *Shigella*/EIEC infections alongside clinical data of the patient and other laboratory test outcomes.

For *in-vitro* professional diagnostic use.

Background

Gastroenteritis is a major cause of morbidity and mortality, worldwide, both in children 5 years old and in the general population.

Campylobacter are gram negative, slender, spirally curved microaerophilic bacteria that live as commensal organisms in the gastrointestinal tract of many domestic and wild birds and mammals. *C. jejuni* and *C. coli* are by far the most important human pathogens in the genus and account for more than 95% of all clinical isolates worldwide.

The genus *Salmonella* contains two distinct species, designated *Salmonella enterica* (divided into six subspecies) and *Salmonella bongori*. *Salmonella* species are a leading bacterial cause of acute gastroenteritis.

Shigellosis produces inflammatory reactions and ulceration on the intestinal epithelium followed by bloody or mucoid diarrhea. It is caused by enteroinvasive *E. coli* (EIEC) as well as any species of the genus *Shigella*, namely, *S. dysenteriae*, *S. flexneri*, *S. boydii*, and *S. sonnei*. Shigellosis is endemic in many developing countries and also occurs in epidemics causing considerable morbidity and mortality.

Principles of the Procedure

The Savvygen™ GI Bacteria Panel test is a ready-to used test, which contains in each well all the necessary reagents for Real-Time PCR assay in a stabilized format. The test is designed for the diagnosis of *Salmonella*, *Campylobacter* and *Shigella*/enteroinvasive *Escherichia coli* (EIEC) in human stool specimens to aid in the assessment of infections caused by these bacteria.

Savvygen™ GI Bacteria Panel test detection is done in a one step Real-Time format where the test is based on the amplification of highly specific conserved fragments of the conserved region of the *invA* gene (*Salmonella*), 16S rRNA gene (*Campylobacter*) and *ipaH* gene (*Shigella*/EIEC). Following extraction of these bacteria's DNA, the conserved fragments are amplified by Taq DNA in a Polymerase Chain Reaction (PCR). The assay is based on the 5'→3' exonuclease activity of Taq DNA Polymerase (figure 1). A fluorophore/quencher dual-labeled probe anneals to an internal specific sequence. Upon primer elongation, Taq DNA Polymerase displaces and hydrolyzes the probe, thus releasing and activating the fluorophore. The presence of GI Bacteria Panel is detected by an increase in observed fluorescence during the reaction. The resulting increase in fluorescence signal is proportional to the amount of amplified product in the sample and detected by the real-time PCR instrument.

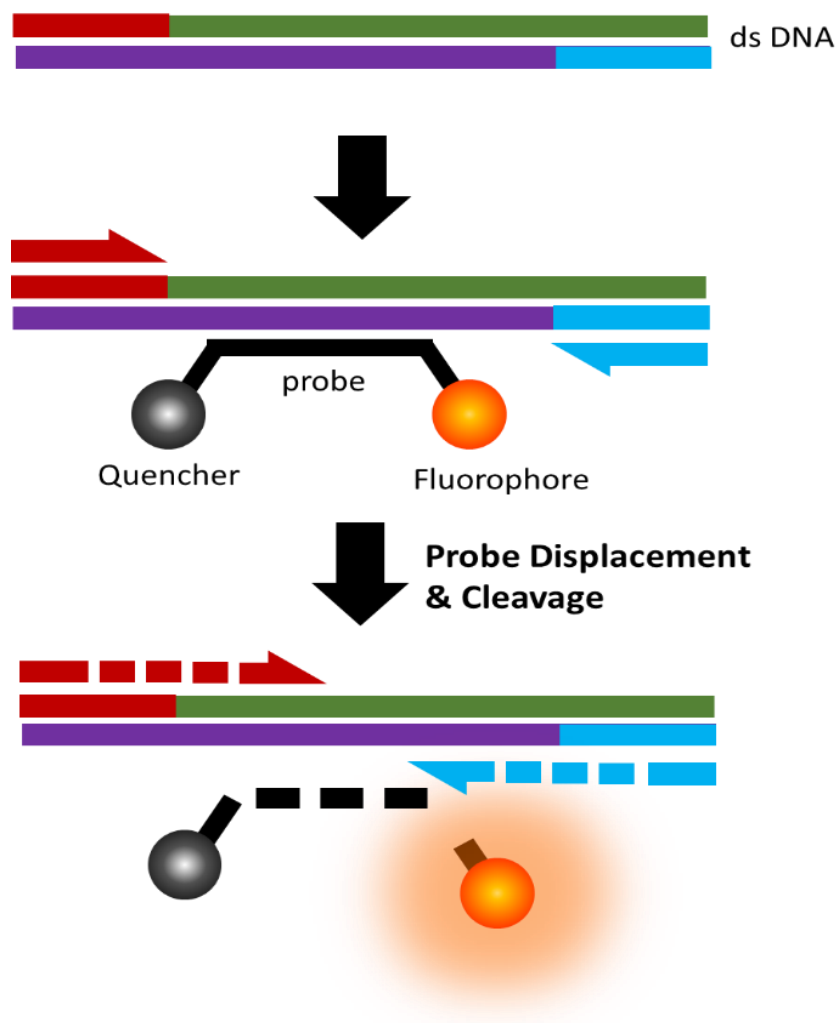


Figure 1. Principle of the Savvygen assay

Savvygen™ GI Bacteria Panel test is a ready-to used test, which contains in each well all the necessary reagents for Real-Time PCR assay in a stabilized format. In addition, an internal control allows the detection of a possible reaction inhibition. The optical channels used for multiplexed detection of the amplified fragments are outlined in Table 1 below:

Table 1. parasites target and optical channel detection;

Target	Optical channel
<i>Salmonella</i>	FAM
<i>Shigella/EIEC</i>	ROX
<i>Campylobacter</i>	Cy5
<i>Internal Control</i>	*HEX, VIC or JOE

Materials/ Reagents Provided

Product Description	Contents
Savvygen™ GI Bacteria Panel 48 reactions. Cat.# 620-01H (High profile) 48 reactions. Cat.# 620-01L (Low profile)	6 x GI Bacteria 8- well strip
	1x GI Bacteria Positive Control (lyophilized)
	1x Water RNase/DNase free 1mL
	1x Rehydration Buffer 1.8 mL
	1x Negative Control 1 mL
	Optical caps

Additional Equipment and Material Required

- DNA extraction kit.
- Centrifuge for 1.5 mL tube.
- Vortex.
- Micropipettes (0.5-20 µL, 20-200 µL).
- Powder-free disposal gloves
- Real-Time PCR instruments (see table 2A+2B for compatible Real-Time PCRs).

Table 2A. Compatible Real-Time PCR instrument (Low-Profile)

Bio-Rad	Applied Biosystems
CFX96 Touch™ Real-Time PCR Detection System	7500 Fast Real-Time PCR System
Roche	7500 Fast Dx Real-Time PCR System
LightCycler®480 Real-Time PCR System	QuantStudio™ 12K Flex 96-well Fast
LightCycler®96 Real-Time PCR System	QuantStudio™ 6 Flex 96-well Fast
Agilent Technologies	QuantStudio™ 7 Flex 96-well Fast
AriaMx Real-Time PCR System	QuantStudio™ 5 Real-Time PCR System
DNA-Technology	ViiA™ 7 Fast Real-Time PCR System
DTlite Real-Time PCR System	Cepheid
DT prime Real-Time Detection Thermal Cycler	SmartCycler®*
	Qiagen
	Rotor-Gen® Q*

Table 2B. Compatible Real-Time PCR instrument (High-Profile)

Bio-Rad	Applied Biosystems
<i>CFX96 Touch Deep Well Real-Time PCR Detection System</i>	<i>7500 Real-Time PCR System</i>
<i>iCycler iQ Real-Time PCR Detection System</i>	<i>QuantStudio™ 12K Flex 96-well</i>
<i>iCycler iQ 5 Real-Time PCR Detection System</i>	<i>QuantStudio™ 6 Flex 96-well</i>
DNA-Technology	<i>QuantStudio™ 7 Flex 96-well</i>
<i>DTlite Real-Time PCR System</i>	<i>QuantStudio™ 5 Real-Time PCR System</i>
<i>DT prime Real-Time Detection Thermal Cycler</i>	<i>ViiA™ 7 Real-Time PCR System</i>
Stratagene /Agilent Technologies	Qiagen
<i>Mx3000P™ Real-Time PCR System</i>	<i>Rotor-Gen® Q*</i>
<i>Mx3005P™ Real-Time PCR System</i>	Cepheid
Analytik Jena Biometra	<i>SmartCycler®*</i>
<i>TOptical</i>	Abbot
<i>qTOWER 2.0</i>	<i>Abbot m2000 RealTime System</i>

* Once the product has been reconstituted following the appropriate procedure, transfer it into the specific Rotor-Gene® Q or SmartCycler® tubes.

Note: Savvygen™ GI Bacteria Panel test has been validated on the following equipment: Applied Biosystems 7500 Fast Real-Time PCR System, Bio-Rad CFX96 Touch™ Real-Time PCR Detection System, Agilent Technologies AriaMx Real-Time PCR System, DNA-Technology DTprime Real-time Detection Thermal Cycler, DNA-Technology DTlite Real-time Detection Thermal Cycler, Rotor-Gene® Q (Qiagen), SmartCycler® (Cepheid),

Transport and Kit Storage

The Savvygen kits can be shipped and stored at 2-37°C until the expiration date stated in the label.


After resuspension of the Positive Control, store at -20°C. Avoid repeated freeze/thaw cycles.

It is recommended to make aliquots of the positive control and store at -20°C once resuspended, in order to avoid freeze & thaw cycles.

Precautions

Amplification technologies can amplify target nucleic acid sequences over a billion-fold and provide a means of detecting very low concentrations of target. Care must be taken to avoid contamination of samples with target molecules from other samples, or amplicons from previous amplifications. Follow these recommendations to help control contamination.

1. Separate pre-amplification steps from post-amplification steps. Use separate locations for pre- and post-amplification. Use suitable lab equipment for each stage. Prepare samples in a laminar flow hood using suitable equipment to minimize contamination. Set up the post-amplification area in a low-traffic area with suitable equipment.

- 
2. The laboratory process must be one-directional, it should begin in the Extraction Area and then move to the Amplification and Detection Areas. Do not return samples, equipment and reagents to the area where the previous step was performed.
 3. Use disposable containers, disposable barrier pipette tips, disposable bench pads, and disposable gloves. Avoid washable lab wear.
 4. Use a diluted bleach solution (0.2% sodium hypochlorite) to treat waste from the post-amplification and detection areas, as the waste contains amplicon. Use the bleach solution to wipe down equipment and bench areas, as well as to treat drains used to dispose of liquid waste.
 5. Use negative controls to monitor for possible contamination during reaction setup. If reagent contamination is detected, dispose of the suspect reagents.
 6. Do not use after expiration date.
 7. Specimens must be treated as potentially infectious as well as all reagents and materials that have been exposed to the samples and handled in the same manner as an infectious agent. Take necessary precautions during the collection, storage, treatment and disposal of samples.

Test Procedure

Positive Control Preparation

Note: *The Positive Control vial contains a high copy number template of the assay targets with a contamination risk. Therefore, it is recommended to resuspend the vial in a separate laboratory area or a special cabinet.*

Open the Positive control pouch to resuspend the lyophilized GI Bacteria Positive Control (tube with red cap) with 100 µL of Water RNase/DNase free (transparent cap vial) supplied. To ensure a complete resuspension, vortex the tube thoroughly. After first use, dispense into aliquots, in order to avoid multiple freeze-thaw cycles, and store them at -20°C.

Specimen Collection, Processing and DNA Extraction

In order to obtain an adequate sample, the procedure for sample collection must be followed closely and according to the manufacturer's instructions. The stool samples should be collected in clean containers and processed as soon as possible to guarantee the quality of the test. However, samples can be frozen at -20°C for long storage. Ensure only the amount needed is thawed because freezing and thawing cycles are not recommended.

Nucleic Acid (NA) Extraction: for pretreatment and NA isolation, it is recommended to use an appropriate DNA extraction kit according to the manufacturer's protocol. NA extraction may be carried out manually or automatically using commercially available extraction kits.

- QIAamp DNA Mini Kit (Qiagen).
- QIAamp DNA Stool Mini Kit (Qiagen).
- Maxwell®RSC Blood DNA Kit, using the Maxwell® 16 instrument (Promega).
- Invisorb® Spin Universal Kit (Strattec).
- RIDA® Xtract (R-biopharm).

PCR protocol program

Set your thermocycler following the conditions below:

Table 3. Real-Time PCR profile

Step	Temperature	Time	Cycles
Polymerase activation	95°C	2 min	1
Denaturation	95°C	10 sec.	45
Annealing/Extension*	60°C	50 sec.	

Note: Set the fluorescence data collection during the extension step (*) through the FAM, ROX, Cy5, and HEX, JOE or VIC channels.

Depending on the equipment used select the proper detection channel (*table 4*). For the Applied Biosystems 7500 Fast Real-Time PCR system or the Stratagene Mx3005P™ Real-Time PCR System check that passive reference option ROX is not marked.

Preparing reaction wells

A. Reconstitute the required reaction wells.

Calculate the number of required reactions including samples and controls. It is highly recommended to run at least one positive and one negative control per run.

1. Peel off protective aluminum seal from the strips/plate.
2. Pipette 15 µL of Rehydration Buffer (Blue cap vial) into each well.

B. Add samples and controls according to real-time PCR experimental plate set up.

1. Pipette 5 µL of DNA sample into each sample well
2. Pipette 5 µL of resuspended GI Bacteria Panel Positive Control (tube with red cap) into the positive control well.
3. Pipette 5 µL of Negative Control (tube with orange cap) into each negative control well.
4. Cover the wells with the caps provided. Spin down briefly if needed.

C. Performing PCR.

1. Place the strips in the Real-Time PCR instrument.
2. Start the run.

The fluorescence detection channels of common Real-Time PCR Thermocyclers are specified in Table 4.

Table 4: Detection fluorescence channels of different Real-Time PCR systems

<i>Real-Time PCR THERMOCYCLER</i>	<i>System Detection channels</i>	<i>Savvygen probes channels</i>	<i>Remarks</i>
Roche LightCycler® 96 or LightCycler®480II	465/510	FAM	Color Compensation is required only for LC480 system
	533/580	HEX	
	533/610	ROX	
	618/660	Cy5	
Applied Biosystems ABI 7500 fast	FAM	FAM	Passive reference option ROX is not mark
	VIC	HEX	
	ROX	ROX	
	Cy5	Cy5	
Bio-Rad CFX96™	FAM	FAM	
	HEX	HEX	
	ROX	ROX	
	Cy5	Cy5	
Agilent AriaMx	FAM	FAM	
	HEX	HEX	
	ROX	ROX	
	Cy5	Cy5	
DNA-Technology DTlite / DTprime	FAM	FAM	
	HEX	HEX	
	ROX	ROX	
	Cy5	Cy5	
Smartcycler® Cepheid	Channel 1	FAM	
	Channel 2	HEX	
	Channel 3	ROX	
	Channel 4	Cy5	
Abbott m2000rt	FAM	FAM	
	HEX	HEX	
	ROX	ROX	
	Cy5	Cy5	
Rotor-Gene®Q Qiagen	Green	FAM	
	Yellow	HEX	
	Orange	ROX	
	Red	Cy5	

Interpretation of results

Interpretation of results can be automatically performed if programmed by the user using the RT-qPCR instrument software following the manufacturer's instructions. It is required to run assay controls (positive and negative controls) in each run to validate the reaction.

Note: The positive controls used in each run, must show an amplification curve for GI Bacteria Panel targets which validates the reaction, while the negative control well should demonstrate an absence of signal (except internal control target).

Table 5: Results interpretation for the Savvygen™ GI Bacteria Panel assay


Interpretation	Salmonella (FAM)	Campylobacter (Cy5)	Shigella (ROX)	Internal control (HEX, VIC or JOE)	Negative control	Positive control
Salmonella, Campylobacter & Shigella/EIEC Positive	POS	POS	POS	POS / NEG	NEG	POS
Salmonella, Campylobacter & Shigella/EIEC Negative	NEG	NEG	NEG	POS	NEG	POS
Campylobacter Positive , Salmonella & Shigella/EIEC Negative	NEG	POS	NEG	POS / NEG	NEG	POS
Salmonella Positive Campylobacter & Shigella/EIEC Negative .	POS	NEG	NEG	POS / NEG	NEG	POS
Shigella/EIEC Positive , Salmonella & Campylobacter Negative .	NEG	NEG	POS	POS / NEG	NEG	POS
Salmonella & Campylobacter Positive , Shigella/EIEC Negative .	POS	POS	NEG	POS / NEG	NEG	POS
Salmonella & Shigella/EIEC Positive , Campylobacter Negative .	POS	NEG	POS	POS / NEG	NEG	POS
Campylobacter & Shigella/EIEC Positive , Salmonella Negative .	NEG	POS	POS	POS / NEG	NEG	POS
Invalid run	POS	POS	POS	POS	POS	POS
Invalid run	NEG	NEG	NEG	NEG	NEG	NEG

POS: presence of Amplification signal

NEG: No amplification signal

Positive sample- A sample is considered a positive for the target if the Ct value is less than 40.

Negative sample- A sample is considered a negative for the target if there is no evidence of amplification signal in the detection system but the internal control is positive.



Internal control- The Internal Controls must show an amplification curve, which verify the correct functioning of the amplification mix. Sometimes, the detection of internal control is not necessary because a high copy number of the pathogen DNA template can cause preferential amplification of target sequence.

Positive control- The positive controls used in each run must show an amplification curve for GI Bacteria Panel, which validates the reaction.

Negative control- The negative controls included in each run, must show the absence of signal for GI Bacteria targets, which validates the reaction.

Invalid run- The assay should be considered as invalid and a new run should be performed if there is signal of amplification for one of the pathogens in the negative control well or absence of signal in the positive control well.

Note: If an amplification curve for the internal control is not shown, the sample should be retested by dilution of the original sample 1:10. Alternatively it is recommended to repeat the nucleic acid extraction due to possible problems caused by PCR inhibitors.

Limitations of the test

- This test provides a presumptive diagnosis of *Salmonella*, *Campylobacter* and *Shigella*/ *enteroinvasive Escherichia coli* (EIEC) pathogens. All results must be interpreted together with other clinical information and laboratory findings available to the physician
- This assay should be used only with fecal samples. The use of other samples has not been established.
- Error results may occur from improper sample collection, handling, storage, technical error, sample mix-up, or because the number of organisms in the sample is below the analytical sensitivity of the test.
- The presence of PCR inhibitors may cause invalid results.
- A false positive result with other targets is possible due to contamination with PCR products from previous testing.
- As with all PCR-based *in-vitro* diagnostic tests, extremely low levels of target below the analytical sensitivity of the assay may be detected, but results may not be reproducible.
- If a certain sample result is Invalid then the sample should be repeated from DNA extraction.

Quality Control

In order to confirm the appropriate performance of the molecular diagnostic technique, an Internal Control (IC) is included in each reaction. This is in addition to the positive and negative controls, in order to interpret the results correctly.

Performance Characteristics

Clinical sensitivity and specificity

A retrospective clinical study of 400 faecal samples from symptomatic patient was conducted to evaluate the performance of the Savvygen™ GI Bacteria Panel test for the detection and differentiation of the enteric bacteria *Salmonella*, *Campylobacter* and *Shigella*/enteroinvasive *Escherichia coli* (EIEC). Clinical specimens were previously characterized by a commercial CE approved kit for the above pathogens- RIDA®GENE Bacterial Stool Panel (r-Biopharm)

The results were as follow: *Salmonella* was detected in 21 out of 21 positive samples by the Savvygen™ GI Bacteria Panel test. One additional sample which obtained a positive indication for *Salmonella* by the Savvygen™ GI Bacteria Panel test, was not detected by the RIDA®GENE test (See table 6).

Campylobacter spp. was detected in 58 positive samples (58/58) by the Savvygen™ GI Bacteria Panel test. 13 additional samples presented positive signals for *Campylobacter* by the Savvygen™ GI Bacteria Panel, while obtaining a negative result by the RIDA®GENE test. . For discrepant analysis, these 13 samples were evaluated by an additional commercial Real-Time PCR ((Mericon-Campylobacter spp Kit; QIAGEN)), which confirmed the Savvygen™ GI Bacteria Panel positive results for the bacteria (See table 6).

Shigella or *EIEC* pathogens were detected in only 1 positive sample by the Savvygen™ GI Bacteria Panel test (See table 6).

Table 6. Results interpretation

Pathogen	Positive Agreement		Specificity	
	TP/ (TP+FN)	Percent	TN/ (TN+FP)	Percent
<i>Salmonella</i>	21/21	100%	378/379	99.7%
<i>Campylobacter</i>	58/58	100%	329/342	96.2%
<i>Shigella/EIEC</i>	1/1	N/A	399/399	100%

The results show a high sensitivity and specificity to detect *Salmonella*, *Campylobacter* and *Shigella* / enteroinvasive *Escherichia coli* (*EIEC*) using the Savvygen™ GI Bacteria Panel test.

Analytical sensitivity

In a series of experiments to establish the limit of detection of the Savvygen™ GI Bacteria Panel for each pathogen, a 10-fold dilution of 10^7 to 10^1 copies/reaction was conducted for each target. According to the results, this assay has a detection limit of ≥ 10 DNA copies per reaction for *Salmonella*, *Campylobacter* and *Shigella* / enteroinvasive *Escherichia coli* (*EIEC*). (Figure 1, 2 and 3).

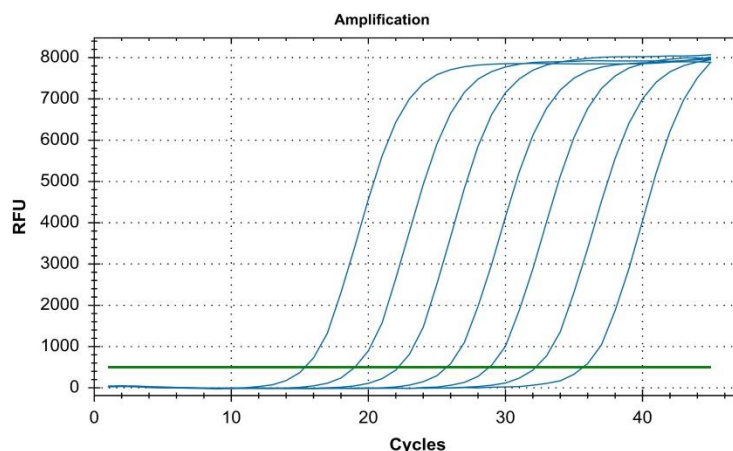


Figure 1. Amplification plot for 10-fold dilution series of *Salmonella* template ranging from 10^7 to 10^1 copies/rxn (FAM channel).

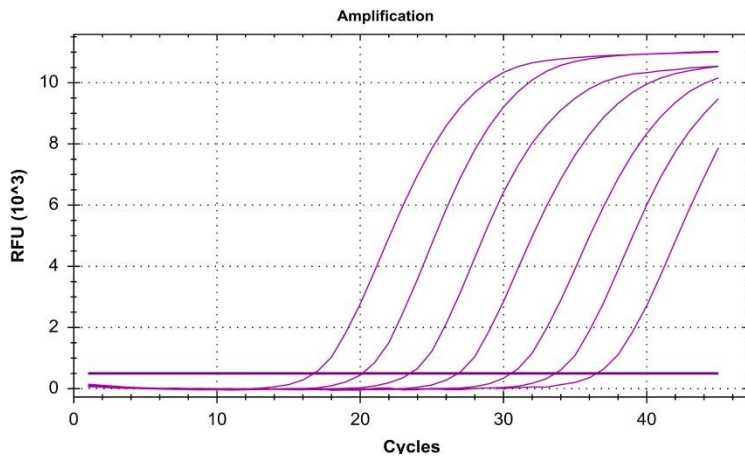


Figure 2. Amplification plot for 10-fold dilution series of *Campylobacter* template ranging from 10^7 to 10^1 copies/rxn (Cy5 channel).

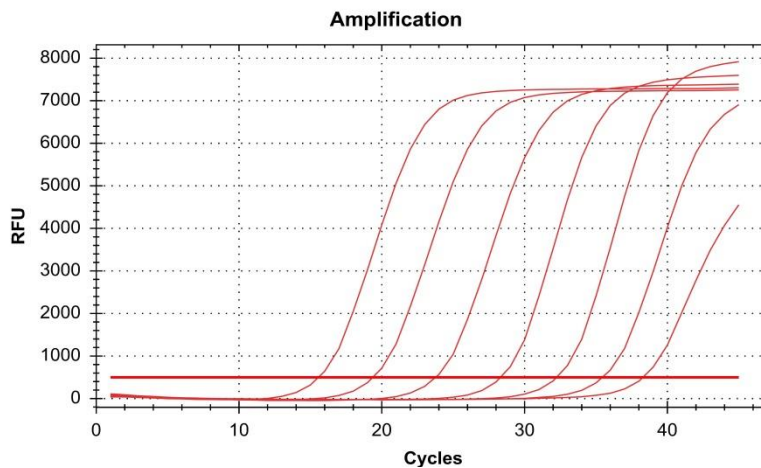


Figure 3. Amplification plot for 10-fold dilution series of *Shigella/EIEC* template ranging from 10^7 to 10^1 copies/rxn (ROX channel).

Analytical specificity

The analytical specificity of the Savvygen™ GI Bacteria Panel for *Salmonella*, *Campylobacter* and *Shigella/EIEC* was evaluated within the panel of following microorganisms. No cross-reactivity was seen between any of the following species (table 7).

Table 7. Cross-reactivity testing.

Pathogen	Cross-Reactivity Test		
	Savvygen™ GI Bacteria Panel		
	<i>Salmonella</i>	<i>Campylobacter</i>	<i>Shigella/EIEC</i>
<i>Adenovirus 40/41</i>	-	-	-
<i>Astrovirus Genotype I-VIII</i>	-	-	-
<i>Norovirus GI and GII</i>	-	-	-
<i>Rotavirus A</i>	-	-	-
<i>Aeromonas hydrophila</i>	-	-	-
<i>Arcobacter butzleri</i>	-	-	-
<i>Bacteroides fragilis</i>	-	-	-

<i>Campylobacter lari</i>	-	N/A	-
<i>Campylobacter fetus</i>	-	N/A	-
<i>Campylobacter coli</i>	-	N/A	-
<i>Campylobacter jejuni</i>	-	N/A	-
<i>Campylobacter upsaliensis</i>	-	N/A	-
<i>Cryptosporidium parvum</i>	-	-	-
<i>Candida albicans</i>	-	-	-
<i>Citrobacter freundii</i>	-	-	-
<i>Clostridium difficile</i>	-	-	-
<i>Clostridium perfringens</i>	-	-	-
<i>Entamoeba histolytica</i>	-	-	-
<i>Enterococcus faecalis</i>	-	-	-
<i>Enterotoxigenic E. coli</i> (ETEC)	-	-	-
<i>Enteropathogenic E. coli</i> (EPEC)	-	-	-
<i>Giardia intestinalis</i>	-	-	-
<i>Helicobacter pylori</i>	-	-	-
<i>Helicobacter hepaticus</i>	-	-	-
<i>Helicobacter cinaedi</i>	-	-	-
<i>Helicobacter heilmannii</i>	-	-	-
<i>Klebsiella oxytoca</i>	-	-	-
<i>Listeria monocytogenes</i>	-	-	-
<i>Pseudomonas aeruginosa</i>	-	-	-
<i>Proteus vulgaris</i>	-	-	-
<i>Salmonella typhi</i>	N/A	-	-
<i>Salmonella paratyphi A</i>	N/A	-	-
<i>Salmonella paratyphi B</i>	N/A	-	-
<i>Salmonella typhimurium</i>	N/A	-	-
<i>Salmonella bongori</i>	N/A	-	-
<i>Salmonella enteritidis</i>	N/A	-	-
<i>Salmonella enterica</i>	N/A	-	-
<i>Salmonella pullorum</i>	N/A	-	-
<i>Salmonella gallinarum</i>	N/A	-	-
<i>Serratia liquefaciens</i>	-	-	-
<i>Shigella flexneri</i>	-	-	N/A
<i>Shigella dysenteriae</i>	-	-	N/A
<i>Staphylococcus aureus</i>	-	-	-
<i>Vibrio parahaemolyticus</i>	-	-	-
<i>Y. enterocolitica</i> O:3 / O:9	-	-	-

Analytical reactivity

The analytical reactivity of the Savvygen™ GI Bacteria Panel test was evaluated with various subtypes of *Salmonella*, *campylobacter* spp. and *Shigella*/EIEC. The tested microorganisms are as listed in table 8:











Table 8. Analytical-reactivity testing.

Pathogen	Analytical-Reactivity Test		
	Savvygen™ GI Bacteria Panel		
	<i>Salmonella</i>	<i>Campylobacter</i>	<i>Shigella</i> /EIEC
<i>Salmonella typhi</i>	+	-	-
<i>Salmonella paratyphi A</i>	+	-	-
<i>Salmonella paratyphi B</i>	+	-	-
<i>Salmonella typhimurium</i>	+	-	-
<i>Salmonella bongori</i>	+	-	-
<i>Salmonella enteritidis</i>	+	-	-
<i>Salmonella enterica</i>	+	-	-
<i>Salmonella pullorum</i>	+	-	-
<i>Salmonella gallinarum</i>	+	-	-
<i>Salmonella mbandaka</i>	+	-	-
<i>Salmonella braenderup</i>	+	-	-
<i>Campylobacter lari</i>	-	+	-
<i>Campylobacter fetus</i>	-	+	-
<i>Campylobacter coli</i>	-	+	-
<i>Campylobacter jejuni</i>	-	+	-
<i>Campylobacter upsaliensis</i>	-	+	-
<i>Campylobacter concisus</i>	-	+	-
<i>Campylobacter hyointestinalis</i>	-	+	-
<i>Campylobacter gracilis</i>	-	+	-
<i>Campylobacter helveticus</i>	-	+	-
<i>Campylobacter curvus</i>	-	+	-
<i>Campylobacter rectus</i>	-	+	-
<i>Shigella dysenteriae</i>	-	-	+
<i>Shigella flexneri</i>	-	-	+
<i>Shigella boydii</i>	-	-	+
<i>Shigella sonnei</i>	-	-	+

Bibliography

1. J. Hoorfar et al. Automated 59 Nuclease PCR Assay for Identification of *Salmonella enterica*. Journal of Clinical Microbiology 2000; 38: 3429–3435.
2. Rodríguez-Lázaro et al. A rapid and direct Real-Time PCR-based method for identification of *Salmonella* spp. Journal of Microbiological Methods 2003; 54: 381– 390.
3. Barletta et al. Multiplex real-time PCR for detection of *Campylobacter*, *Salmonella*, and *Shigella*. Journal of Clinical Microbiology 2013; 51: 2822-2829.
4. N.O. Kaakoush et al. Global Epidemiology of *Campylobacter* Infection. Clinical Microbiology Reviews 2015; 28(3): 687-720.
5. S.M. Man. The clinical importance of emerging *Campylobacter* species. Nature Reviews Gastroenterology & Hepatology 2011; 8(12): 669-685.
6. R.F. de Boer et al. Detection of *Campylobacter* species and *Arcobacter butzleri* in stool samples by use of realtime multiplex PCR. Journal of Clinical Microbiology 2013; 51(1): 253-259.
7. N. Botteldoorn et al. Quantification of *Campylobacter* spp. in chicken carcass rinse by real-time PCR. Journal of Applied Microbiology 2008; 105(6):1909-1918.
8. A.Ub-Din et al. Relationship among *Shigella* spp. and *enteroinvasive Escherichia coli* (EIEC) and their differentiation. Brazilian Journal of Microbiology 2014; 45(4): 1131-1138.
9. V. D. Thiem et al. Detection of *Shigella* by a PCR assay targeting the ipaH gene suggests increased prevalence of shigellosis in Nha Trang, Vietnam. Journal of Clinical Microbiology 2004; 42(5): 2031-2035.
10. W. S. Lin et al. A quantitative PCR assay for rapid detection of *Shigella* species in fresh produce. Journal of Food Protection 2010; 73(2): 221-233.
11. W. Mokhtari et al. Real-Time PCR using SYBR Green for the detection of *Shigella* spp. in food and stool samples. Molecular and Cellular Probes 2013; 27: 53-59.
12. S. Ghosh et al. Genetic characterization of *Shigella* spp. isolated from diarrhoeal and asymptomatic children. Journal of Medical Microbiology 2014; 63: 903-910.

Symbols for IVD Components and Reagents

	Manufacturer		Use by		For <i>in vitro</i> diagnostic use only
	Lot number		Temperature limitation		Consult instructions for use
	Catalogue number		Contains sufficient for <n> test		Buffer (sample diluent)
	Keep Dry				

CFX™ and IQ5™ are registered trademarks of Bio-Rad Laboratories.

ABI®, QuantStudio™, StepOnePlus™ and ViiA™ are registered trademarks of Thermo Fisher Scientific Inc.

LightCycler® is a registered trademark of Roche.

Mx3000P™ and Mx3005™ are registered trademarks of Agilent Technologies.

Rotor-Gene® Q is a registered trademark of Qiagen.

SmartCycler® is a registered trademark of Cepheid