



SZABO SCANDIC

Part of Europa Biosite

Produktinformation



Forschungsprodukte & Biochemikalien



Zellkultur & Verbrauchsmaterial



Diagnostik & molekulare Diagnostik



Laborgeräte & Service

Weitere Information auf den folgenden Seiten!
See the following pages for more information!



Lieferung & Zahlungsart

siehe unsere [Liefer- und Versandbedingungen](#)

Zuschläge

- Mindermengenzuschlag
- Trockeneiszuschlag
- Gefahrgutzuschlag
- Expressversand

SZABO-SCANDIC HandelsgmbH

Quellenstraße 110, A-1100 Wien

T. +43(0)1 489 3961-0


F. +43(0)1 489 3961-7

mail@szabo-scandic.com

www.szabo-scandic.com


[linkedin.com/company/szaboscandic](https://www.linkedin.com/company/szaboscandic) 

Cytation™ 5 Cell Imaging Multi-Mode Reader

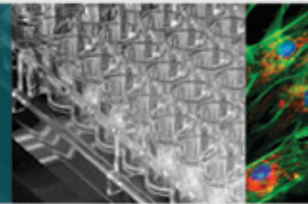


Cytation™ 5 is a uniquely integrated, configurable instrument that combines automated digital widefield microscopy with conventional multi-mode microplate detection to provide phenotypic cellular information and well-based quantitative data. Cytation 5 replaces multiple modules and software interfaces, yet is simple to setup and operate. With up to 60x magnification, the microscopy module provides high-quality cellular and sub-cellular visualization in fluorescence, brightfield, color brightfield and phase contrast modes. Patent pending laser autofocus and image-based autofocus provide rapid, accurate methods for a wide variety of


samples. The multi-mode detection module features BioTek's patented Hybrid Technology™, which incorporates variable bandwidth monochromator optics and high sensitivity filter-based detection optics for unmatched versatility and performance. Temperature control to 65 °C and shaking, plus available CO₂/O₂ control and dual reagent injectors optimize conditions for cell-based imaging and detection. Image capture, data collection and powerful image and data analysis are managed with Gen5™ Microplate Reader and Imager Software, specifically designed for uncomplicated processing of even the most complex assays.

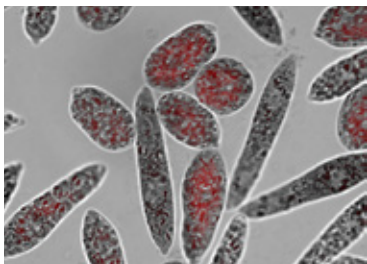


Euglena gracilis, 60x

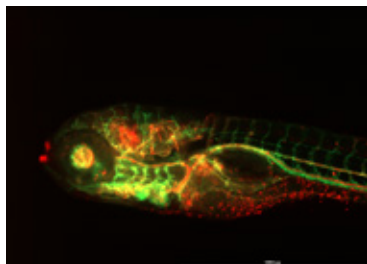

Zebrafish, 4x

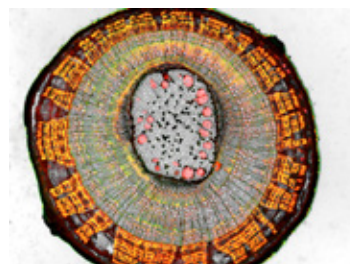

TiliaStem, 2x

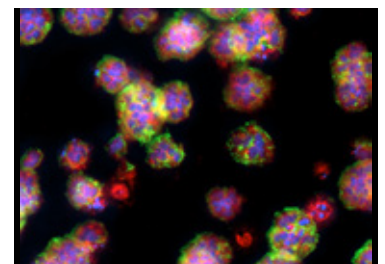

Z-stack, 20x



Cytation 5 with dual injector and CO₂/O₂ Gas Controller

Features:

- Fluorescence, brightfield, color brightfield and phase contrast microscopy and conventional multi-mode detection
- Patent pending laser autofocus provides speed and accuracy
- Label-free cell counting for cell proliferation assays
- Patented Hybrid Technology™ in multi-mode detection combines high performance filters with variable bandwidth monochromators for versatility and performance
- Variable bandwidth fluorescence monochromators offer a 9 nm to 50 nm in 1 nm increments for ultimate flexibility
- Laser-based excitation for Alpha assays
- CO₂/O₂ control, incubation to 65 °C and shaking optimize cell-based and other assays
- Low volume (2 µL) nucleic acid and protein quantification with the available Take3 Plates
- Powerful yet easy to use Gen5 software for efficient plate reading, image capture and analysis
- BioSpa™ 8 Automated Incubator compatible for live and fixed cell assays automation

Typical Applications:

- 2D and 3D cell imaging and analysis
- Cell proliferation
- Cytotoxicity
- Label-free cell counting
- Color brightfield imaging
- Protein expression
- Biomarker quantification
- Drug discovery
- Genetic analysis
- Drug absorption and metabolism
- Biologics drug discovery and development
- Environmental testing
- Food safety
- Nucleic acid quantification
- Protein quantification

Configurations:

CYT5PV:	Cytation 5 w/imaging
CYT5MFV:	Cytation 5 w/imaging, monochromator fluorescence and UV-Vis absorbance, filter-based fluorescence
CYT5MV:	Cytation 5 w/imaging, monochromator fluorescence and UV-Vis absorbance
CYT5MFA:	Cytation 5 w/imaging, monochromator fluorescence and UV-Vis absorbance, laser Alpha
CYT5M:	Cytation 5 w/monochromator fluorescence

Note: Several other configurations are available. Ask your BioTek Sales Representative or visit www.biotek.com for details.

Optional Accessories:

- Joystick Controller
- CO₂/O₂ Gas Controller Module
- Dual Reagent Injector Module
- BioStack™ Microplate Stacker
- BioSpa™ 8 Automated Incubator
- Take3™ Micro-Volume Plate
- Gen5™ Secure for 21 CFR part 11 compliance
- Luminescence, Fluorescence and Absorbance Test Plates
- Gen5 Image+ Software
- High Contrast Brightfield kit for Label-free Cell Counting



Cytation 5 interfaces with the BioSpa 8 Automated Incubator for live cell assay workflows.

"Alpha" refers to products/technologies from PerkinElmer, Inc., that carry trademarks or registered trademarks.



BioTek Instruments, Inc.
Highland Park, P.O. Box 998
Winooski, Vermont 05404-0998, USA

Phone: 802-655-4040 • Toll-Free: 888-451-5171
Outside the USA: 802-655-4740

www.biotek.com

Specifications:

General

Imaging modes:	Fluorescence, brightfield, phase contrast, color brightfield
Detection mode:	Monochromators: FL, Lum., UV-Vis Abs., TRF (secondary) Filters: FL, TRF, FP, Lum., Alpha
Read method:	End point, kinetic, well mode, time-lapse, montage
Labware type:	6- to 384-well plates, microscope slides, Petri dishes, cell culture flasks (T25) Take3™ Micro-Volume Plates
Temperature control:	4-Zone™ incubation to 65 °C with Condensation Control™ Variation: ±0.2 °C at 37 °C
Shaking:	Linear, orbital, double orbital
Automation:	BioStack™ and 3rd party automation compatible BioSpa™ 8 Automated Incubator compatible
CO ₂ and O ₂ control:	Optional Gas Controller available
Software:	Gen5™ Microplate Reader and Imager Software included; Gen5 Image+ software available for full image analysis

Imaging

Light source:	High power LEDs (available wavelengths: 365 nm, 390 nm, 465 nm, 505 nm, 523 nm, 590 nm, 623 nm, 655 nm, 740 nm)
Camera:	16-bit gray scale, Sony CCD, 1.1 megapixel
Filter cube capacity:	4 user-replaceable fluorescence cubes plus brightfield channel
Objective capacity:	6 objectives turret
Available objectives:	Fluorescence: 1.25x, 2.5x (2.25x eff), 2.5x (2.75x eff), 4x, 10x, 20x, 40x, 60x Phase contrast: 4x, 10x, 20x, 40x
Image collection rate:	96 wells, 1 color (DAPI), 4x, 6 minutes 96 wells, 3 colors, 4x, 12 minutes
Resolution:	0.3µm/pixel at 20x
Automated functions:	Autofocus, autoexposure, auto-LED intensity
Autofocus methods:	Patent pending laser autofocus; image-based autofocus

Fluorescence Intensity

Sensitivity:	Monochromators: Top: Fluorescein 2.5 pM (0.25 fmol/well 384-well plate) Bottom: Fluorescein 4 pM (0.4 fmol/well 384-well plate) Filters/mirrors: Fluorescein 0.25 pM (0.025 fmol/well 384-well plate)
Light source:	Xenon flash lamp
Wavelength selection:	Double grating monochromators (top and bottom) Deep blocking bandpass filters/dichroic mirrors (top)
Wavelength range:	Monochromators: 250 – 700 nm (850 nm option) Filters: 200 – 700 nm (850 nm option)
Dynamic range:	7 decades
Detection system:	Two PMTs: (1) for monochromator system, (1) for filter system

Luminescence

Sensitivity:	Monochromators: 20 amol ATP (flash); Filters: 10 amol ATP (flash)
Wavelength range:	300 – 700 nm
Dynamic range:	>6 decades

Fluorescence Polarization

Sensitivity:	1.2 mP standard deviation at 1nM fluorescein
Wavelength range:	280 – 700 nm (850 nm option)

Time-Resolved Fluorescence

Sensitivity:	Europium 40 fM with filters (4 amol/well in 384-well plate) Europium 1200 fM with monos (120 amol/well in 384-well plate)
Light source:	Xenon flash lamp
Wavelength range:	Monos: 250 – 700 nm (850 nm option) Filters: 200 – 700 nm (850 nm option)

Absorbance

Light source:	Xenon flash lamp
Wavelength selection:	Monochromator
Wavelength range:	230 – 999 nm, 1 nm increment
Bandpass:	4 nm (230 – 285 nm), 8 nm (>285 nm)
Dynamic range:	0 – 4.0 OD

Alpha Detection

Light source:	680 nm laser, 100 mW +/-10%
Wavelength selection:	Filter (top only)
Sensitivity:	100 amol LCK peptide (384-well low volume plate)

Reagent Dispensers

Number:	2 syringe pumps
Dispense volume:	5 – 1,000 µL in 1 µL increment
Dead volume:	1.1 mL, 100 µL with back flush
Plate geometry:	6- to 384-well microplates
Dispense precision:	<2% at 50 – 200 µL
Dispense accuracy:	±1 µL or 2%

Performance values represent the average observed factory test values.

*Specifications subject to change.

Rev. 132SS060617